


Figure 1: Coverage of the Putamen with VY-AADC01

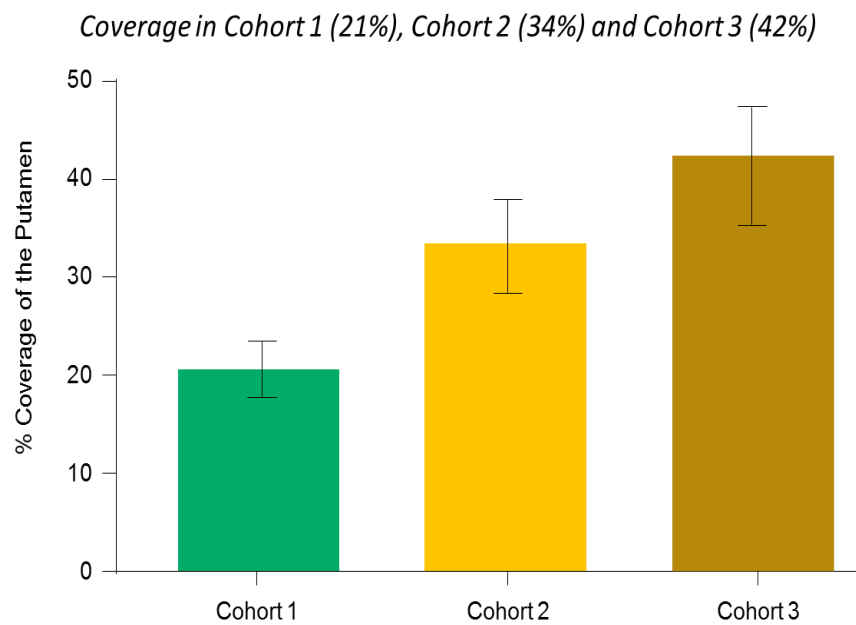

Note: % coverage of the putamen represents average coverage of left and right putamen by volume. Error bars are standard deviations.
Source: Voyager Therapeutics, Inc.
